



# UPO1000HD Series

## High-Resolution Oscilloscopes

### Data Sheet

V1.0

Apr. 2025

## Product Introduction

High-Resolution 1000HD series high-resolution oscilloscope has the maximum bandwidth of 150 MHz, the maximum sampling rate of 1.25 GSa/s, and is equipped with 4/2 analog channels, with the memory depth of up to 100 Mpts. High-Resolution 1000HD series adopts exclusive Ultra Phosphor 3.0 technology, achieving the waveform capture rate of up to 100,000 wfms/s, with 256 levels of gray temperature colors, and features an innovative digital trigger system with high trigger sensitivity and low jitter.

This oscilloscope supports multiple advanced triggers, serial bus triggering and decoding, and offers advanced sampling and analysis modes such as spectrum analysis, power analysis, histogram, waveform recording, hardware-accelerated template testing, and search and navigation.


Additionally, this oscilloscope provides multiple measurements and mathematical operations.

High-Resolution 1000HD series features a 7-inch capacitive touch screen that supports multiple gestures for common waveform operations. Combined with multiple one-touch keys on the front panel, this greatly optimizes the efficiency of oscilloscope operation and improves the user experience.



# Mainstream Touchscreen Design Providing Intelligent Interactive Experience

Featuring a 7-inch HD capacitive multi-touch screen, it supports a variety of gesture operations such as touch, drag, zoom and rectangle drawing. This makes operation more convenient and smoother, and helps the user learn the instrument more easily. It retains the traditional key and knob operation while also supporting mouse and keyboard, making instrument operation more versatile and greatly improving the interactive experience.

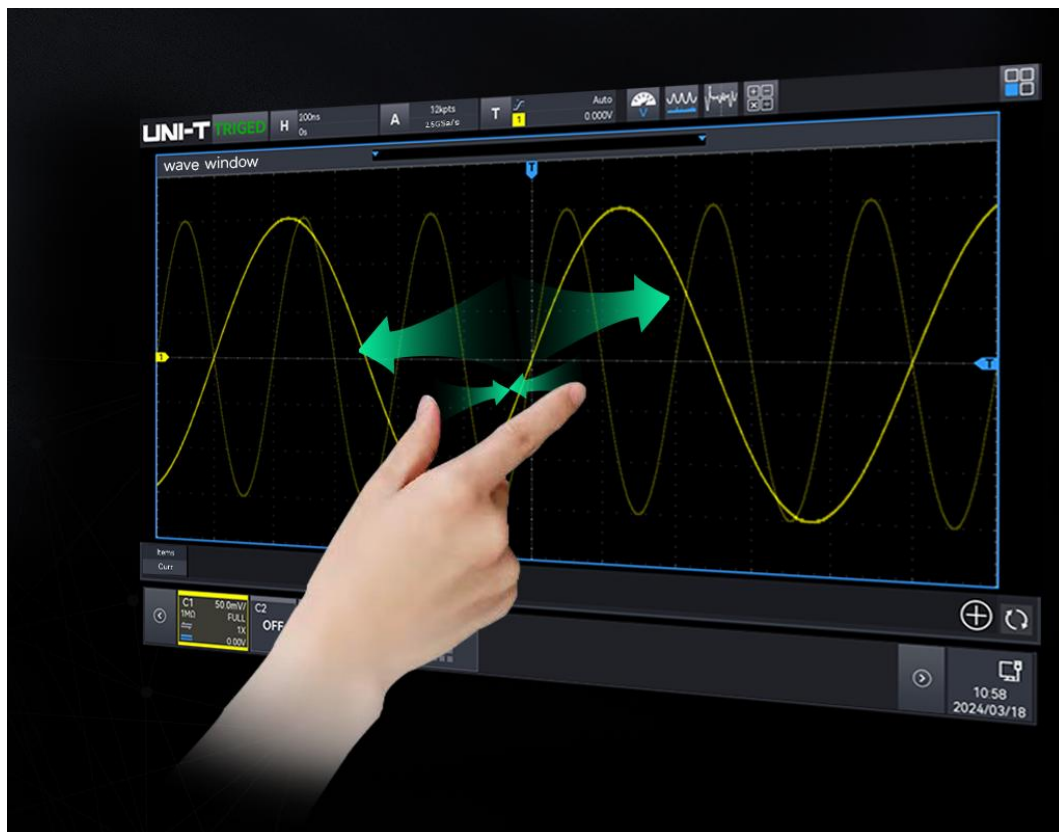

## Brand New Appearance Design

High-Resolution 1000HD series features an innovative appearance with a double-sided thinning design. The display is aligned horizontally with the panel to enhance touch operation and visibility range. The black frame margin, enhances the overall sense of the instrument.



## Features and Advantages


- Analog channel bandwidth: 150 MHz/80 MHz
- Real-time sampling rate of the analog channel is up to 1.25 GSa/s.
- 12-bit vertical resolution, with up to 4096 points, ensures that the waveform details are clearly visible.
- 4/2 analog channels and the memory depth of up to 100 Mpts
- The maximum waveform capture rate is up to 100,000 wfms/s (sequence mode: 1,000,000 wfms/s)
- 7 instrument functions: Digital oscilloscope, logic analyzer, spectrum analyzer, digital voltmeter, frequency meter, protocol analyzer, and power analyzer.
- Parameter measurement adds Bar Chart and line graph display
- Uninterrupted hardware real-time waveform recording and analysis of up to 100,000 frames and supports USB memory export function.
- Enhanced FFT of up to 1M points, supporting the spectrum analyzer functions such as frequency setting, waterfall curve, detection setting, and marker.
- 56 kinds of parameter measurements
- Multi-Windows display
- Multi-channel 6-digit hardware frequency meter, supporting frequency refresh time and adjustable effective digit settings.
- DVM multi-channel RMS measurement: DC, AC RMS, and DC+ACRMS
- Multiple trigger types: Edge, pulse width, video, ramp, runt pulse, over-amplitude pulse, delay, timeout, duration, setup & hold, Nth edge and, code pattern
- Protocol triggering and decoding function: RS232/UART, I<sup>2</sup>C, SPI, CAN, LIN
- Zone trigger for capturing sporadic signals and observing complicated signals.
- Ultra Phosphor3.0 provides a super fluorescent display effect with up to 256 levels of gray.
- 7-inch 1024x600 HD capacitive multi-touch screen, supporting gesture control such as click, slide, zoom, edit, and drag
- Multiple peripheral interfaces: USB Host, USB Device, LAN, AUX Out (Trig Out, Pass/Fail, DVM), HDMI
- Supports SCPI (Standard Command for Programmable Instrument)
- Built-in WebServer for accessing and controlling the instrument through a browser, supporting access from PC and mobile devices for cross-platform compatibility.
- Supports on-line update



# Design Features

## High-resolution


12-bit high-resolution ADC sampling has a quantization level of up to 4096, which is 16 times that of a traditional 8-bit ADC, allowing for better restoration of waveform details.

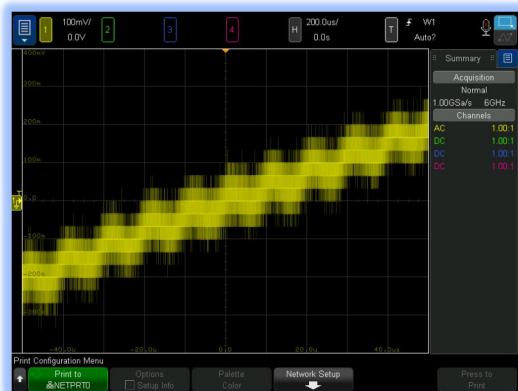

8-bit




12-bit

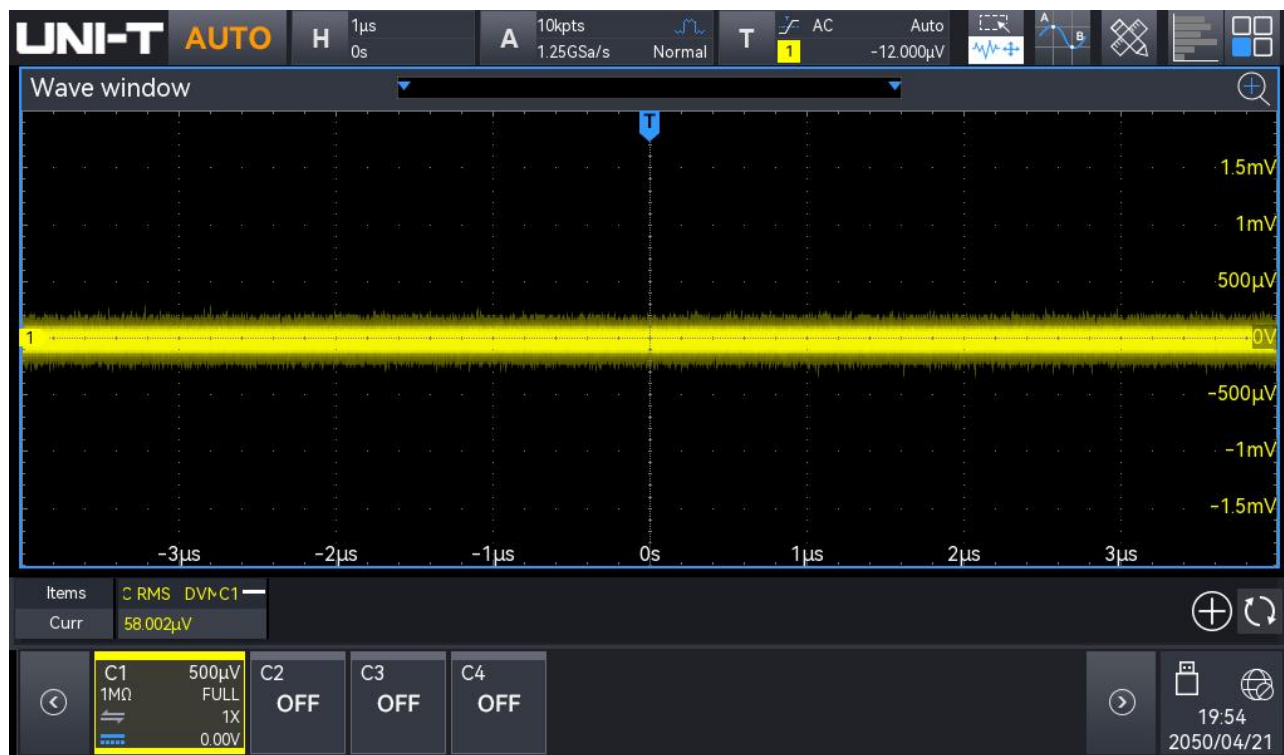


The excellent background noise, which is only 60  $\mu\text{Vrms}$  at the full bandwidth of 150 MHz, allows the 12-bit ADC to perform optimally.

## Application Scope

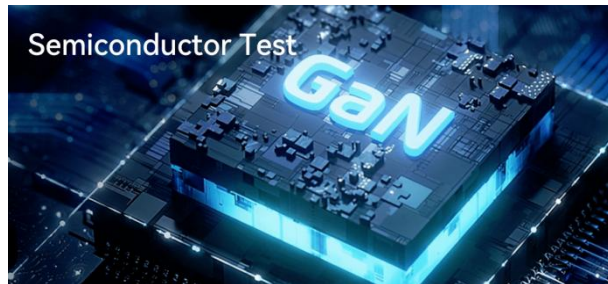


## Cost-effective, Nine-in-one Integrated Oscilloscope

High-Resolution 1000HD series integrates nine instrument functions, including a digital oscilloscope, logic analyzer, spectrum analyzer, digital voltmeter, high-precision frequency meter, protocol analyzer, and power analyzer. This is a cost-effective oscilloscope for users.

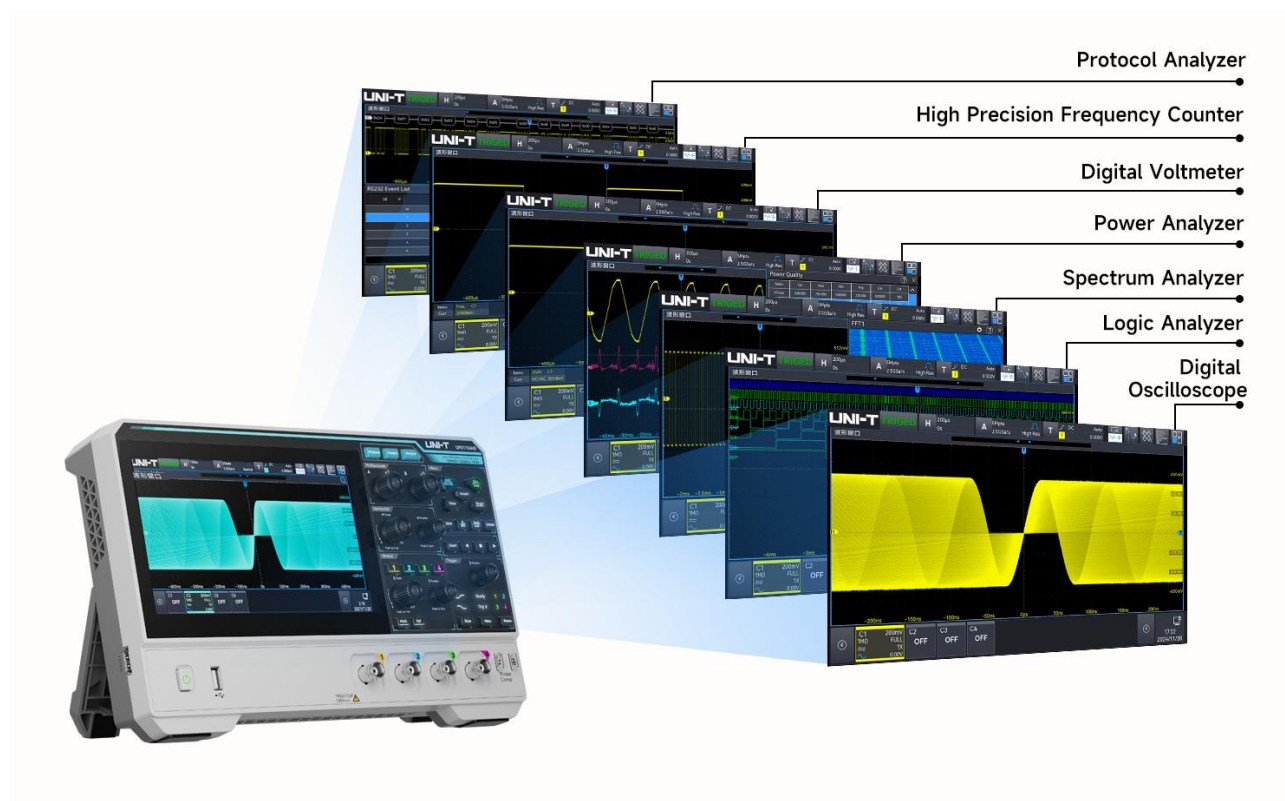

## Digital Oscilloscope

- Bandwidth: 150 MHz/80 MHz
- Maximum real-time sampling rate: 1.25 GSa/s
- Maximum memory depth: 100 Mpts
- 4 analog channels

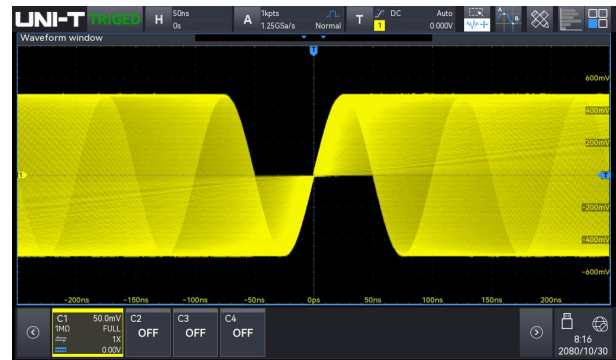

## Spectrum Analyzer

- Standard enhanced FFT with up to 1 Mpts for 4-channel signal analysis
- Frequency range: 0 to 625 MHz
- Waterfall curve
- 4 traces and 4 detections
- Mark type: Auto, manual and threshold
- Marker point list



## Digital Voltmeter

- 4-digit voltmeter
- Measurement: DC/AC RMS/AC+DC RMS
- Limit alarm



## High-precision Frequency Meter


- 6-digit hardware frequency meter
- Frequency meter: Refresh time and adjustable effective digit settings
- Summary counter





## Protocol Analyzer

- 5 kinds of triggering and decoding protocols, including those for computers, embedded serial buses, automobile, and audio applications.
- Decoding can be operated in the pause and record modes.
- Supports event list and search function

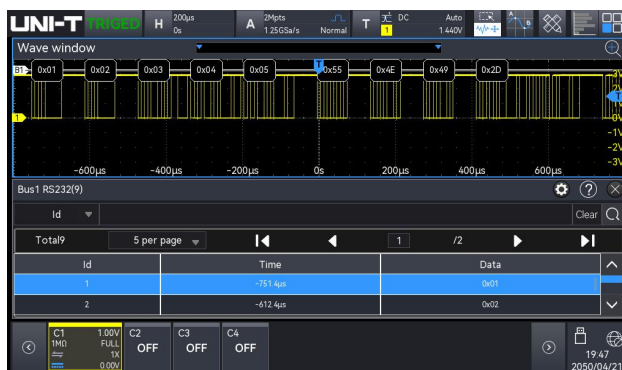


Name	Description	Standard
Computer serial bus triggering and analysis	RS-232/422/485/UART	Standard
Embedded serial bus triggering and analysis	I <sup>2</sup> C, SPI	Standard
Automobile serial bus triggering and analysis	CAN	Standard
Automobile serial bus triggering and analysis	LIN	Standard

## Power Analyzer

With the development of chip technology, the requirements for power supply systems are also increased. Nowadays, low-voltage, high-current power supply networks have become a trend. Especially for chips or networks composed of precision components, it is essential to ensure reliable power supply and noise suppression across various parts of the circuit, as well as to maintain the integrity of signal transmission between chips. This presents greater challenges for power supply testing. Designers are now more focused on energy-efficient power supplies and response speed to ensure the power supply remains stable and clean. Based on this, power integrity testing becomes particularly important. Power integrity directly affects signal integrity, and conversely, signal quality also reflects power quality. Furthermore, power quality can cause a series of electromagnetic interference issues, which can be a significant concern for designers. Therefore, having an oscilloscope capable of power analysis is undoubtedly your best choice.

High-Resolution 1000HD series provides a comprehensive set of power analysis tools and evaluation results. To use them, simply select the appropriate analysis type and connect the voltage probe and current probe to the power system test point or specified test fixtures, as shown in the diagram. Then, connect to the desired channel for observation and make any necessary fine-tuning adjustments to achieve your desired results.

- Power quality
- Harmonic analysis
- Current harmonics
- Rds (on)
- Switching loss
- Conversion rate
- Safe operating area
- Modulation analysis
- Output ripple
- Startup/shutdown time
- Transient response \*
- Power efficiency \*

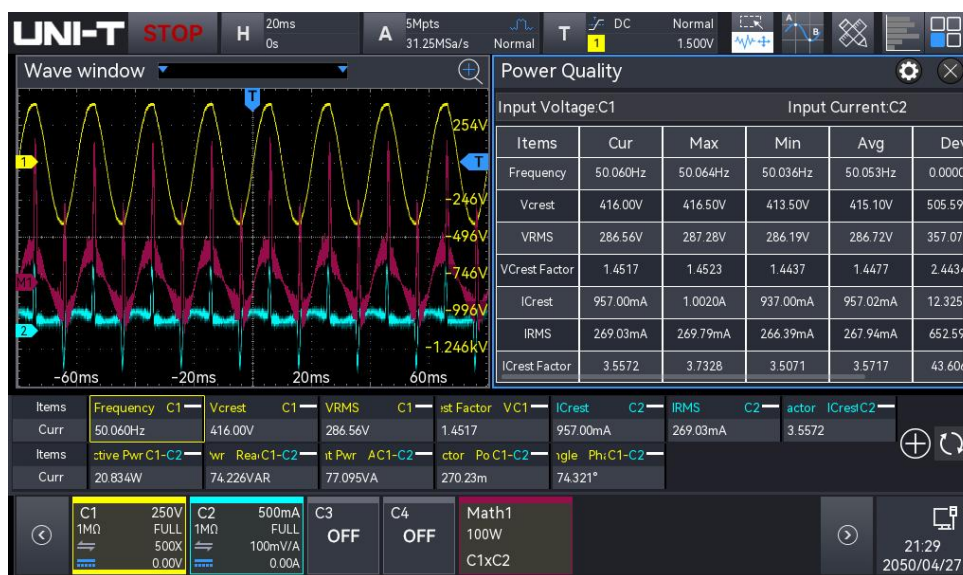


“\*” indicates features being added. Power analysis support is subject to the latest firmware available on the official website.

## Ultra Phosphor 3.0

When attempting to identify and debug occasional or intermittent anomalies in signals, the waveform capture rate is a crucial indicator. This rate represents the oscilloscope's ability to capture waveforms per unit of time, reflecting its speed in processing and analyzing signals.

High-Resolution 1000HD series uses advanced software and hardware architecture to achieve 5 to 10 times higher data processing performance than previous generation products. Equipped with Ultra Phosphor 3.0, it supports serial graphics mapping, with a processing rate of up to 20 Gbps and the waveform capture rate of up to 100,000 wfms/s, and up to 1 million 2.2 ns fast edge signals in sequence mode, facilitating easy and accurate capture of occasional signals.

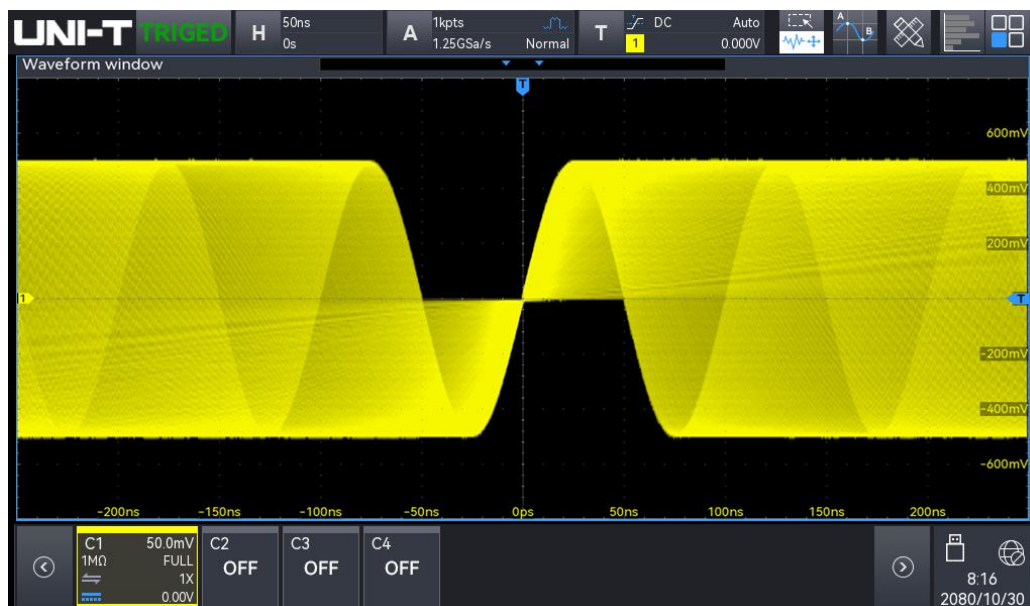

## Brand New Quick Autoset Strategy

Fuzzy control is an intelligent control method based on fuzzy set theory, fuzzy linguistic variables, and fuzzy logic reasoning. The advantages of the algorithm are fewer iterations, faster speed, and better anti-interference ability.

In the past, oscilloscopes performed Autoset to find the appropriate signal amplitude and frequency for display. However, the response speed varied significantly among oscilloscope manufacturers due to different solutions adopted. This inconsistency affected the user experience.

UNI-T has redefined Autoset execution by adopting a fast fuzzy algorithm based on analog signals and multi-channel parallel processing technology. This is complemented by a 7-bit high-precision hardware frequency counter, allowing the oscilloscope to quickly find and process the amplitude and frequency of unknown signals during Autoset execution. The entire channel can be opened in less than 1.5s, and a single channel in less than 1s, greatly enhancing working efficiency and reducing the risk of misuse for users who frequently change test objects and require rapid testing.

## Type-C for Power Supply

High-Resolution 1000HD series adopts the latest Type-C power supply method. When no power source is available outdoors, it can be powered by a portable charger.



## Wall-mounted Interface

In a crowded laboratory or other limited-space environments, the wall-mounting option provides a more convenient and flexible way to use High-Resolution 1000HD series without occupying valuable workspace. The wall-mounted interface on the rear panel measures 100 mm x 100 mm.

## Multiple Parameter Measurements

Parameter measurement is a crucial function for engineers when using an oscilloscope.

High-Resolution 1000HD series provides 56 measurement parameters, with the capability to display up to 21 measurement parameters simultaneously. Each page of measurement statistics displays 7 parameters, which can be presented in histograms and trend charts. The histogram visually represents the probability distribution of the parameters, while the trend chart reflects parameter changes over time.

The parameter snapshot displays 39 test items for single-channel measurement. These include voltage and time measurement parameters, with measured results constantly refreshed during the process. High-Resolution 1000HD series introduces a new amplitude calculation strategy, incorporating both top and bottom measurement methods. Parameters related to RMS (root mean square), burst, setup, and hold can be configured, making it easier for engineers to utilize the




parameter measurement function and enabling accurate, real-time analysis of channel measurement data.



## Mathematical Operation

High-Resolution 1000HD series provides a system of algorithms for complex waveform operations, allowing you to further process waveforms and display the results directly on the oscilloscope.

- Basic operation: +, -, \*, ÷
- Digital filter: High-pass, low-pass, band-pass, and band-limit
- Custom function operation: Analog channel and Math waveform

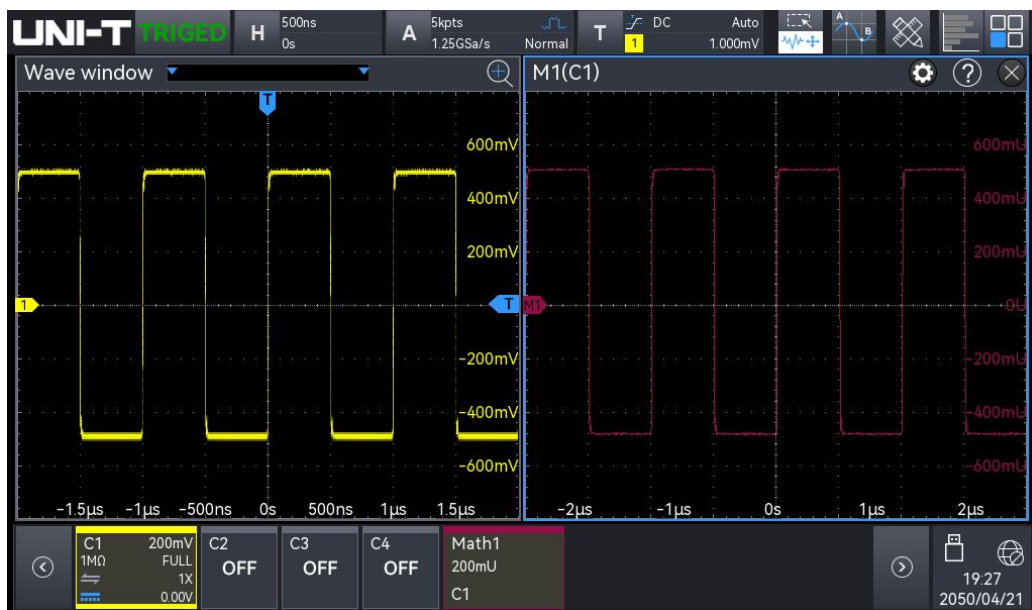

## Navigation and Search


The memory depth of High-Resolution 1000HD series is 100 Mpts, allowing it to capture tens of thousands of waveforms in one capture. Searching for waveforms manually can be time-consuming for engineers.

High-Resolution 1000HD series provides customizable search conditions, which are very useful for locating sampled signals and finding waveforms of interest. With the analysis function, events can be analyzed in detail, eliminating the time-consuming and inconvenient process of manual searches.



## Hardware-accelerated Template Test

Using hardware-accelerated template testing, the waveform test can be completed in a few seconds to meet special standards.

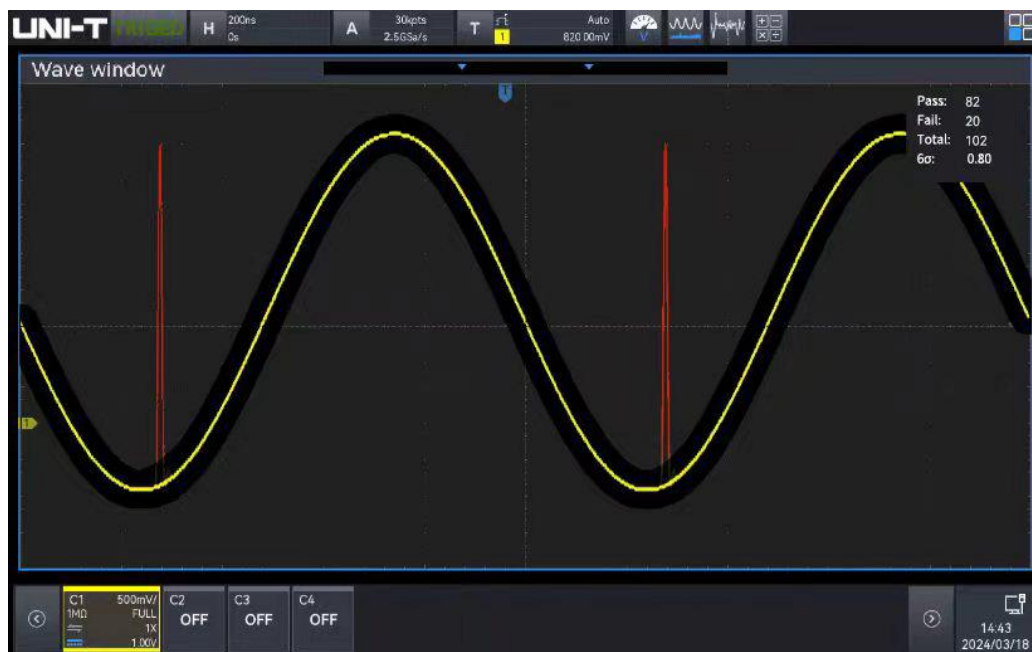

## Zone Trigger


The zone trigger function serves two purposes: firstly, to isolate occasional abnormal signals, and secondly, to stabilize the waveform display. Only a stable trigger can provide a stable waveform display. With this function, engineers can handle complex and variable signals during debugging. The zone trigger function is easy to use, so engineers don't have to spend time learning how to use it.

A rectangle drawing gesture can quickly isolate a signal to be observed. The waveform does not have to be completely stable to trigger; the zone trigger function can capture a waveform that meets the specified conditions and stabilize it for triggering.



## Various Connection

High-Resolution 1000HD series offers a wide range of connections with flexibility and convenience.

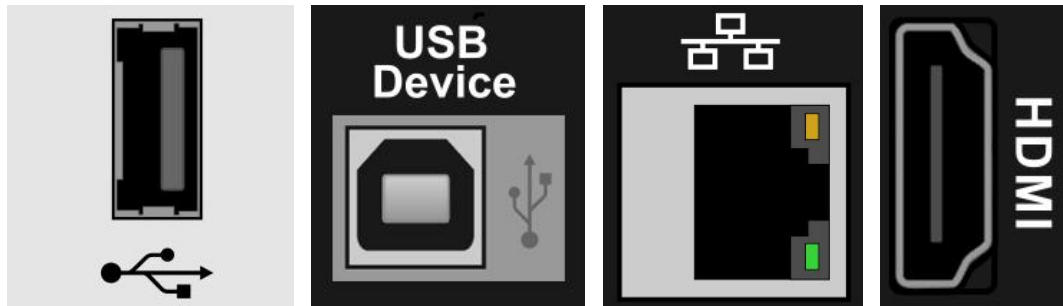

## Multiple Control Methods

Control or secondary development through the instruction set conforming to the SCPI standard.

```
def test_square_character(dst_instr, src_instr, image_list, sheet_list, test_para, show_changeChannel1234_9800T):
    test_para['AutoTest'] = True
    dst_instr.write("*RST")
    src_instr.write("*RST")
    time.sleep(3)
    dst_instr.write(":ACQ:TYPE AVER")
    dst_instr.write(":ACQ:AVER:COUN 8")
    time.sleep(1)
    data = dst_instr.query("SYSTem:INFORM")
    strArray = data.split(',')
    channelNumbers = 4
    for i in range(channelNumbers):
        srcChannelNumber = i + 1
        dstChannelNumber = i + 1
        channelName = 'CH{0}'.format(dstChannelNumber)
        src_instr.write(":CHANnel{0}:BASE:WAVE SQUARE".format(srcChannelNumber))
        src_instr.write(":CHANnel{0}:OUTPUT 1".format(srcChannelNumber))
        dst_instr.write(":CHAN{0}:DISP ON".format(dstChannelNumber))
        time.sleep(1)
        dst_instr.write(":CHAN{0}:COUP DC".format(dstChannelNumber))
        dst_instr.write(":WAVEform:SOURce CHAN{0}".format(dstChannelNumber))
        dst_instr.write(":WAVEform:MODE NORMAL")
        dst_instr.write(":WAVEform:FORMat BYTE")
        for amp,vbase in zip(amps, vbases):
            src_instr.write(":CHANnel{0}:BASE:AMPLitude {1}".format(srcChannelNumber, amp))
            time.sleep(0.5)
            dst_instr.write("TRIGger:SOURce CHANnel{0}".format(dstChannelNumber))
            dst_instr.write("CHAN{0}:SCAL {1:.6f}V".format(dstChannelNumber, vbase))
            time.sleep(0.1)
        for freq,timeBase,precision in zip(freqs, times, precisions):
            if(freq <= 100):
```



## Use UNI-T free instrument manager for control.

It can be controlled by installing instrument management software on the PC side through LAN or USB Device.



## WebServer

SCPI for remote checking and control

Export waveform files

Browsing the user manual online

PC/Mobile phone access



# Document Version and Revision

Document Version	V1.0
Document Revision	Original version
Firmware version: V1.00.0024   Logic version: V1.00.0006   Hardware version: V1.02.0000	

## Performance Characteristics

All specifications are guaranteed, except those marked "Typical (Typ.)".

Unless otherwise stated, all the performance characteristics are suitable for the probe attenuation ratio is set to 10x and High-Resolution 1000HD series high-resolution oscilloscopes.

To meet these specifications, the oscilloscope should first meet the following conditions.

- The instrument must be operated continuously for at least thirty minutes at the specified operating temperature.
- The self-calibration must be performed when the operating temperature reaches or exceeds 5 °C.

Model	UPO1152HD	UPO1154HD	UPO1082HD	UPO1084HD
Analog bandwidth	150 MHz		80 MHz	
Calculated rise time (10 to 90%) (typical)	≤2.2 ns		≤4 ns	
Input/output channel number	2 analog channels	4 analog channels	2 analog channels	4 analog channels
Sampling mode	Real-time sampling			
Acquisition mode	Normal, peak detect, high resolution, averaging			
Maximum sample rate	Analog channel: 1.25 GSa/s (single channel), 625 MSa/s (dual channels), 312.5 MSa/s (four channel)			
Average	After all channels have reached N samples simultaneously, the number of N times can be selected from 2, 4, 8, 16, 32, 64, 128, 256, 512, 1024, 2048, 4096, 8192.			
Memory depth	Auto (limit to 5 Mpts), 25 kpts, 250 kpts, 500 kpts, 5 Mpts, 50 Mpts, 100 Mpts			
Maximum waveform capture rate	100,000 wfms/s 1,000,000 wfms/s (sequence mode)			
Sequential sampling	Maximum 100,000 frames, minimum two trigger intervals < 1000 ns			
Hardware real-time waveform recording and playing	100,000 frames			
Screen	7 - inch 1024x600 HD capacitive touch screen			
Vertical System (Analog channel)				
Input coupling	DC, AC, GND			
Input impedance	(1 MΩ ± 2%)    (17 pF ± 2 pF)			
Probe attenuation factor	Voltage probe ratio: 0.001X, 0.01X, 0.1X, 1X, 10X, 100X, 1000X, Custom Current probe ratio: 5 mV/A, 10 mV/A, 50 mV/A, 100 mV/A, 200 mV/A, 500			

	mV/A, 1V/A, Custom
Maximum input voltage	400 V (DC+ACVpk) 135 V <sub>RMS</sub>
Vertical resolution	12-bit (ERES is enabled with a maximum of 16-bit)
Vertical scale	500 $\mu$ V/div to 10 V/div
Offset range	500 $\mu$ V/div to 50 mV/div: $\pm 2$ V 51 mV/div to 1 V/div: $\pm 25$ V 1.02 V/div to 10 V/div: $\pm 250$ V Vertical offset reading: V
Band limit (typical)	20 MHz, Full
Low-frequency response	(AC coupling, -3 dB); $\leq 5$ Hz (on BNC)
DC gain accuracy	$< 5$ mV: $\pm 2\%$ full scale, $\geq 5$ mV: $\pm 1.5\%$ full scale
DC offset accuracy	$\pm (2\% + 0.1 \text{ div} + 2 \text{ mV})$
Unit	W, A, V, and U, default: V
Channel-to-channel isolation(typical)	DC to maximum bandwidth: $> 40$ dB

### Horizontal System (Analog channel)

	2 ns/div to 1 ks/div	5 ns/div to 1 ks/div
Time base range	(simultaneously display the current sampling rate and memory depth)	(simultaneously display the current sampling rate and memory depth)
Time base accuracy	$\pm 25$ ppm	
Time base delay time range	Pre-trigger (negative delay): $\geq 1$ screen width Post-trigger (positive delay): 1 s to 4 ks	
	Y-T (default)	
	X-Y (CH1-CH2, CH1-CH3, CH1-CH4, CH2-CH3, CH2-CH4, CH3-CH4)	
Time base mode	Roll, time base $\geq 50$ ms/div, using the horizontal rotary knob to enter or exit Roll mode	
	Scan, time base $\geq 50$ ms/div, user can select Roll or Scan mode	

### Trigger

	CH1-CH4:
Trigger Sensitivity	$\leq 10$ mV/div, The larger value of 1div or 5 mVpp $> 10$ mV/div, 0.5 div
	Enable the noise rejection, with trigger sensitivity reducing half
	Trigger sensitivity can be customized, with the default set to 50%
Trigger level range	Internal: $\pm 4$ div from the center of the screen
Trigger modes	Auto, Normal, Single



Trigger holdoff range	0.0 ps to 10 s
Trigger coupling (Typ.)	DC: Allows all signals to pass
	AC: Blocks the DC component of the input signal
	HF reject: Suppresses high-frequency components of signals above 40 kHz
	LF reject: Suppresses low-frequency components of signals below 40 kHz
Noise reject	Suppress the high-frequency noise of signal, to reduce the error-touched possibility Enable the noise rejection, with trigger sensitivity reducing half
<b>Zone Triggering</b>	
Zone	2 zones; source: CH1-CH4; Feature: Must Intersect, Must Not Intersect
<b>Edge</b>	
Slope	Rising, Falling, Either
Source	CH1-CH4
<b>Runt</b>	
Trigger condition	>, <, ≤, ≥, None
Polarity	Positive, Negative
Pulse width	6.4 ns to 10 s
Source	CH1-CH4
<b>Window</b>	
Polarity	Rising, Falling, Either
Trigger condition	Enter, Exit, Time
Set	6.4 ns to 10 s
Source	CH1-CH4
<b>Nth edge</b>	
Slope	Rising, Falling
Idle time	6.4 ns to 10 s
Edge number	1 to 65535
Source	CH1-CH4
<b>Delay</b>	
Edge type	Rising, Falling
Trigger condition	>, <, ≤, ≥, > <
Delay time	6.4 ns to 10 s
Source	CH1-CH4
<b>Timeout</b>	
Slope	Rising, Falling, Either

Timeout	6.4 ns to 10 s
Source	CH1-CH4
<b>Duration</b>	
Code pattern	H, L, X
Trigger condition	>, <, ≤ ≥
Duration	6.4 ns to 10 s
Source	CH1-CH4
<b>Setup and Hold</b>	
Clock edge	Rising, Falling
Data type	H, L
Setup	6.4 ns to 10 s
Hold	6.4 ns to 10 s
Source	CH1-CH4
<b>Pulse Width</b>	
Polarity	Positive, Negative
Trigger condition	>, <, ≤ ≥
Pulse Width	1.6 ns to 4 s
Source	CH1-CH4
<b>Slope</b>	
Slope	Positive, Negative
Trigger condition	>, <, ≤ ≥
Time	3.2 ns to 1 s
Source	CH1-CH4
<b>Video</b>	
Standard	PAL, NTSC, SECAM, 525 p/60, 625 p/50, 720 p/24, 720 p/25, 720 p/30, 720 p/50, 720 p/60, 1080 i/25, 1080 i/30, 1080 p/24, 1080 p/25, 1080 p/30, 1080 pfs/24
Source	CH1-CH4
<b>Pattern</b>	
Code pattern	H, L, X, Rising, Falling
Source	CH1-CH4
<b>RS232/UART</b>	
Trigger condition	Start, StopBit, CheckErrr, Data
Baud rate	2400 bps, 4800 bps, 9600 bps, 19200 bps, 38400 bps, 57600 bps, 115200 bps, custom
Data bit	5 bits, 6 bits, 7 bits, 8 bits

Source	CH1-CH4
--------	---------

**I<sup>2</sup>C**

Trigger condition	Start, Restart, Stop, Loss, Address, Data, Address & Data
-------------------	---

Addr mode	7 bits, 10 bits
-----------	-----------------

Addr range	0 to 7F, 0 to 3 FF
------------	--------------------

Byte length	1 to 5
-------------	--------

Source	CH1-CH4
--------	---------

**SPI**

Mode	Timeout, CS
------	-------------

Trigger condition	Start, Data
-------------------	-------------

Timeout	99.2 ns to 1 s
---------	----------------

Data bit	4 bits to 32 bits
----------	-------------------

Source	CH1-CH4
--------	---------

**CAN**

Signal type	CAN_H, CAN_L
-------------	--------------

Trigger condition	Start, Data Frame, Remote Frame, Error Frame, Over-Load, Identifier, Data, Identifier&Data, End of Frame, Missing Ack, Biterror, CRC, Error, ALL Errors
-------------------	---

Data rate	10 kbps, 19.2 kbps, 20 kbps, 33.3 kbps, 38.4 kbps, 50 kbps, 57.6 kbps, 62.5 kbps, 83.3 kbps, 100 kbps, 115.2 kbps, 125 kbps, 230.4 kbps, 250 kbps, 490.8 kbps, 500 kbps, 800 kbps, 921.6 kbps, 1 Mbps, 2 Mbps, 3 Mbps, 4 Mbps, 5 Mbps, custom
-----------	---

Source	CH1-CH4
--------	---------

**LIN**

Trigger condition	Sync, Identifier, Data, Identifier & Data, Wake Frame, Sleep Frame, Error
-------------------	---

Version	v1.x, v2.x, Either
---------	--------------------

Baud rate	1.2 kbps, 2.4 kbps, 4.8 kbps, 9.6 kbps, 10.417 kbps, 19.2 kbps, 20 kbps, custom
-----------	---

Data length	1 to 8
-------------	--------

Source	CH1-CH4
--------	---------

**Decoding**

Number of decodes	4
-------------------	---

Decoding type	Standard: RS232/UART, I2C, SPI CAN, LIN
---------------	---

Source	CH1-CH4
--------	---------

**Measurement**

Cursor	Voltage difference between cursors ( $\Delta Y$ )
	Time difference between cursors ( $\Delta X$ )
	Reciprocal of $\Delta X$ (Hz) ( $1/\Delta X$ )

	Voltage and time of waveform point
	Display the cursor in the automatic measurement
Automatic measurements	<b>Analog channel: 56 kinds of parameter</b> Maximum, Minimum, Top, Base, Amplitude, Middle, Peak-Peak, Average, Average-Cycles, RMS, RMS-Cycles, AC RMS, AC RMS-Cycles, Area, Area-Cycles, +Area, -Area, +Area-Cycles, -Area-Cycles, +Overshoot, -Overshoot, +Preshoot, -Preshoot, Period, Frequency, Rise time, Fall time, +Width, -Width, +Duty, -Duty, +Pulse count, -Pulse count, Rising edge count, Falling edge count, Burst width, Burst Interval, Burst Period, Burst Per count, Ratio, Period Ratio, Setup time, Hold time, Setup & Hold Ratio, FRFR, FRFF, FFFR, FFFF, FRLF, FRLR, FFLR, FFLF, Delay(r-r), Delay(f-f), Phase(r-r), Phase(f-f)
Measurement mode	Common measurement and accuracy measurement (Full memory hardware measurements)
Measurement type	Simultaneously display 21 kinds of parameter measurement
Measurement range	Main time base, Zoom time base, Cursor area
Measurement statistics	Mean, Maximum, Minimum, Std Dev, Count, Tendency chart, Bar Chart
XY measurement	Time, Cartesian, Polar, Product, Ratio
Analysis	Frequency Counter, DVM, Pass/Fail, Waveform recording, Power Analysis
<b>Power Analysis</b>	
Measure	Power quality, Current harmonics, Surge current, Rds(on), Switching Loss, Conversion rate, Safe operating area, Modulation analysis, Output ripple, Startup/shutdown time, Transient response, Power efficiency
<b>Histogram</b>	
Source	CH1 to CH4
Type	Horizontal, Vertical
<b>Math</b>	
Waveform math	A+B, A-B, A×B, A÷B, Advanced, Filter
Filter	Low pass, High pass, Band pass, Band stop
Operation	0,1,2,3,4,5,6,7,8,9 (+, -, *, /, ^, >, <, &&,   , ==, !=)
Function	sin, cos, sinc, tan, sqrt, exp, lg, ln, floor, abs, acos, asin, atan, sinh, tanh, ceil, cosh, fabs, intg, diff, sign
<b>FFT</b>	
Channel number	4
Window types	Hanning, Hamming, Rectangle, Blackman
FFT count	Up to 1 Mpts



FFT vertical scale	Vrms, dB
	Waterfall: ON, OFF
FFT	Spectrum range: Start frequency, Stop frequency, Center frequency, Span
	Four traces: Normal, Average, Max Hold, Min Hold
	Marker: Marker type, Marker Points, Marker list

### Storage

Setting	Set Status (.set)
Waveform	Waveform data (*.dat) (*.csv) (*.bsv)
Image	Image storage (*.bmp) (*.png) (*.jpg)
Report	Decoding Event List (*.csv) (*.pdf) (*.html)

### DVM (typical)

Source	Analog channel
Mode	DC, AC+DC RMS, AC RMS
Resolution	4-bit
Buzzer	Beeps when the specified limit values are reached or exceeded

### Frequency Counter

Source	Any analog channel
Measurement	Frequency, Period, Totalizer
Counter	The maximum effective digits are 6, and the refresh time and effective digits are adjustable.
Maximum measurement frequency	Maximum bandwidth of analog channel
Time reference	Internal reference: $\pm 25$ ppm

### Interface

USB-Host 2.0	1 on the front panel
USB-Device 2.0	1 on the rear panel
LAN	LAN (VXI11), 10/100 Base-T, RJ-45
AUX Out	Trig Out, Pass/Fail, DVM
HDMI <sup>1</sup>	1 port for external display or projector

### General technical specification

#### Probe compensator output

Output voltage	3 Vpp
Frequency	10 Hz ,100 Hz, 1 kHz (default), 10 kHz

#### Power Source

Power source	Power is greater than or equal to 12 V/3 A
--------------	--

voltage	Supports Type-C or a portable charger with PD protocol
Power consumption	65 W Max
Fuse	1.6 A

### Environmental

Temperature	Operating: 0°C to +40°C
	Non-operating: -20°C to +60°C
Cooling	Forced cooling by fan
Humidity	Operating: below +35 °C, relative humidity ≤90%
	non-operating: +35 °C to +40 °C, relative humidity ≤60%
Altitude	Operating: below 3,000 meters; non-operating: below 15,000 meters
Pollution degree	2
Operating environment	In-door

### Mechanical Specifications

Dimension (W×H×D)	282 mm×175 mm×49 mm
Weight	1.56 kg

### Calibration interval

Calibration interval	1 year
----------------------	--------

### Safety Regulations

Compliance with EMC directive (2014/30/EU), compliance with or superior to IEC 61326-1:2021/ EN61326-1:2021, IEC 61326-2-1:2021/ EN61326-2-1:2021

Electromagnetic compatibility	Conducted disturbance	CISPR 11/EN 55011	CLASS B group 1, 150 kHz-30 MHz
	Radiation disturbance	CISPR 11/EN 55011	CLASS B group 1, 30 MHz-1 GHz
	(ESD)	IEC 61000-4-2/EN 61000-4-2	4.0 kV (contact), 8.0 kV (air)
	Radio sensitivity	IEC 61000-4-3/EN 61000-4-3	0V/m (80 MHz to 1 GHz) 3V/m (1.4 GHz to 2 GHz) 1V/m (2.0 GHz to 2.7GHz)
	Electrical fast transient (EFT)	IEC 61000-4-4/EN 61000-4-4	2kV (AC input)
	Surge	IEC 61000-4-5/EN	1kV (live to zero) 2kV (live/zero to ground)

	61000-4-5	
	IEC	
Radio continuous sensitivity	61000-4-6/EN 61000-4-6	3V, 0.15-80 MHz
		Voltage dip: 0% UT during 1 cycle 40% UT during 10/12 cycles 70% UT during 25/30 cycles Short-term interruption: 0% UT during 250/300 cycles
Voltage dip and short-term interruption	IEC 61000-4-11/EN 61000-4-11	
Safety specification	EN 61010-1:2010+A1:2019 EN IEC61010-2-030:2021+A11:2021 UL61010-1:2012 Ed.3+ R:19 Jul2019 UL61010-2-030:2018 Ed.2 CSA C22.2#61010-1:2012 Ed.3+U1;U2;A1 CSA C22.2#61010-2-030:2018 Ed.2	

## Remarks

1: only support standard HDMI, not support other adapters.

## Order Information





	Description	Order No.
Model	UPO 1152HD (150 MHz, 2 analog channels)	UPO 1152HD
	UPO 1154HD (150 MHz, 4 analog channels)	UPO 1154HD
	UPO 1082HD (80MHz, 2 analog channels)	UPO 1082HD
	UPO 1084HD (80MHz, 4 analog channels)	UPO 1084HD
Standard accessories	National standard cable x 1	
	USB2.0 cable x 1	UT-D14
	Passive probe (200MHz/100MHz) (4/2)	UT-P05/ UT-P04
Optional accessories	Isolation transformer	UT-ISOT
	Deskew Fixture	UT-DF01
	High voltage probe	UT-V23/UT-P21/UT-P20
	High voltage differential probe	UT-P30/UT-P31/UT-P32/ UT-P33/UT-P35/UT-P36
	Current probe	UT-P40/UT-P41/UT-P42/ UT-P43/UT-P44/UT-P4030D/UT-P 4150/UT-P4500/P4100A/P4100B

Remarks: Please order all hosts, accessories and options from your local UNI-T distributor.



## Passive Probe





Instruments.uni-trend.com




<b>UT-P08A</b> 	High resistance probe	10X: DC to 350 MHz Input resistance: 10 M $\Omega$ Maximum operating voltage: < 600V pk Oscilloscope compatibility: All UNI-T series
<b>UT-P20</b> 	High resistance probe	DC to 100 MHz Probe coefficient 100:1 Maximum operating voltage: 1500 Vrms Oscilloscope compatibility: All UNI-T series
<b>UT-V23</b> 	High voltage probe	DC to 100 MHz Probe coefficient 100:1 Input resistance: 100 M $\Omega$ $\pm$ 2% Maximum operating voltage: 2000 Vpp Oscilloscope compatibility: All UNI-T series
<b>UT-P21</b> 	High voltage probe	DC to 50 MHz Probe coefficient 1000:1 Maximum operating voltage: DC 15 kVrms, AC 10 kV (sine wave) Oscilloscope compatibility: All UNI-T series


## Current Probe

Model	Type	
<b>UT-P40</b> 	Current probe	DC to 100 kHz Range: 50 mV/A, 5 mV/A Current range: 0.4 A to 60 A Maximum operating voltage: 600 Vrms Oscilloscope compatibility: All UNI-T series
<b>UT-P41</b> 	Current probe	DC to 100 kHz Range: 100 mV/A, 10 mV/A Current range: 0.4 A to 100 A Maximum operating voltage: 600 Vrms Oscilloscope compatibility: All UNI-T series

UT-P42		Current probe	DC to 150 kHz Range: 100 mV/A, 10 mV/A Current range: 0.4 A to 200 A Maximum operating voltage: 600 Vrms Oscilloscope compatibility: All UNI-T series
UT-P43		Current probe	DC to 25 MHz Range: 100 mV/A Maximum test current: 20 A Rising time: 14 ns Oscilloscope compatibility: All UNI-T series
UT-P44		Current probe	DC to 50 MHz Range: 50 mV/A Maximum test current: 40 A Rising time: 7 ns Oscilloscope compatibility: All UNI-T series
UT-P4030D		High-frequency current probe	Bandwidth: DC to 100 MHz Rising time: $\leq 3.5$ ns Range selection: 30 A/5 A Maximum test current: 30 A Voltage of insulated line: 300 V CAT I Oscilloscope compatibility: All UNI-T series
UT-P4150		High-frequency current probe	Bandwidth: DC to 12 MHz Rising time: $\leq 29$ ns Range selection: 150 A/30 A Maximum test current: 150 A Voltage of insulated line: 600 V CATII 300 V CATIII Oscilloscope compatibility: All UNI-T series
UT-P4500		High-frequency current probe	Bandwidth: DC to 5 MHz Rising time: $\leq 70$ ns Range selection: 500 A/75 A Maximum test current: 500 A Voltage of insulated line: 600V CATII 300 V CATIII

		Oscilloscope compatibility: All UNI-T series
UT-P4100A		Bandwidth: DC to 600 kHz Rising time: $\leq 583$ ns Maximum test current: 100 A Range selection: 100 A/10 A Range sensitivity: 0.1 V/A, 0.01 V/A Common-mode voltage RMS: CATI 600 V CATII 600 V CATIII 300 V Oscilloscope compatibility: All UNI-T series
UT-P4100B		Bandwidth: DC to 2 MHz Rising time: $\leq 175$ ns Maximum test current: 100 A Range selection: 100 A/10 A Range sensitivity: 0.1 V/A, 0.01 V/A Common-mode voltage RMS: CATI 600 V CATII 600 V CATIII 300 V Oscilloscope compatibility: All UNI-T series

## Active Probe

Model	Type	
UT-P30		DC to 100 MHz Attenuation ratio 100:1,10:1 Input differential-mode voltage: $\pm 800$ Vpp Oscilloscope compatibility: All UNI-T series
UT-P31		DC to 100MHz Attenuation ratio 1000:1,100:1 Input differential-mode voltage: $\pm 1.5$ kVpp Oscilloscope compatibility: All UNI-T series

## UT-P32



High voltage  
differential  
probe

DC to 50 MHz  
Attenuation ratio 1000:1,100:1  
Input differential-mode voltage:  $\pm 3$  kVpp  
Oscilloscope compatibility: All UNI-T series

## UT-P33



High voltage  
differential  
probe

DC to 120 MHz  
Attenuation ratio 100:1,10:1  
Input differential-mode voltage:  $\pm 14$  kVpp  
Oscilloscope compatibility: All UNI-T series

## UT-P35



High voltage  
differential  
probe

DC to 50 MHz  
Attenuation ratio 500:1,50:1  
Rising time: 7 ns  
Accuracy: 2%  
Input differential-mode voltage:  
1/50:130 (DC+peakAC)  
1/500:1300 (DC+peakAC)  
Input common-mode voltage:  
100 Vrms, CATI  
600 Vrms, CATII  
Oscilloscope compatibility: All UNI-T series

## UT-P36



High voltage  
differential  
probe

DC to 50 MHz  
Attenuation ratio 2000:1,200:1  
Rising time: 3.5 ns  
Accuracy: 2%  
Input differential-mode voltage:  
1/200:560 (DC+peakAC)  
1/2000:5600 (DC+peakAC)  
Input common-mode voltage:  
2800 Vrms, CATI  
1400 Vrms, CATII  
Oscilloscope compatibility: All UNI-T series

## Options Ordering and Installation

1. **Purchase options:** Based on your requirements, please purchase the specified function options from UNI-T Sales Personnel and provide the serial number of the instrument that needs the option installed.
2. **Receive certificate:** You will receive the license certificate based on the address provided in the order.
3. **Register and obtain license:** Visit the UNI-T official website license activation session for registration. Use the license key and instrument serial number provided in the certificate to obtain the option license code and license file.
4. **Install the option:** Download the option license file to the root directory of a USB storage device and connect the USB storage device to the instrument. Once the USB storage device is recognized, the Option Install menu will be activated. Press this menu key to begin installing the option.



## Limited Warranty and Liability

Uni-T guarantees that the Instrument product is free from any defect in material and workmanship within three years from the purchase date. This warranty does not apply to damages caused by accident, negligence, misuse, modification, contamination, or improper handling. If you need a warranty service within the warranty period, please contact your seller directly. Uni-T will not be responsible for any special, indirect, incidental, or subsequent damage or loss caused by using this device. For the probes and accessories, the warranty period is one year. Visit [instrument.uni-trend.com](http://instrument.uni-trend.com) for full warranty information.



Learn more at: [www.uni-trend.com](http://www.uni-trend.com)



Register your product to confirm your ownership. You will also get product notifications, update alerts, exclusive offers and all the latest information you need to know.

**UNI-T** is the licensed trademark of UNI-TREND TECHNOLOGY (CHINA) CO., Ltd.

UNI-T products are protected under patent laws in China and internationally, covering both granted and pending patents. Licensed software products are the properties of UNI-Trend and its subsidiaries or suppliers, all rights reserved. This manual contains information that replaces all earlier published versions. The product information in this document subject to update without notice. For more information on UNI-T Test & Measure Instrument products, applications, or service, please contact UNI-T instrument for support, the support center is available on [www.uni-trend.com](http://www.uni-trend.com) -> [instruments.uni-trend.com](http://instruments.uni-trend.com)

<https://instruments.uni-trend.com/ContactForm/>

### Headquarter

UNI-TREND TECHNOLOGY (CHINA)  
CO., Ltd.  
Address: No.6, Industrial North 1st  
Road, Songshan Lake Park, Dongguan  
City, Guangdong Province, China  
Tel: (86-769) 8572 3888

### Europe

UNI-TREND TECHNOLOGY EU GmbH  
Address: Affinger Str. 12  
86167 Augsburg Germany  
Tel: +49 (0)821 8879980

### North America

UNI-TREND TECHNOLOGY US  
INC.  
Address: 3171 Mercer Ave STE 104,  
Bellingham, WA 98225  
Tel: +1-888-668-8648